

## A robotic assistant for trans-oral surgery: the robotic endo-laryngeal flexible (Robo-ELF) scope

Kevin Olds · Alexander Hillel · Jonathan Kriss · Archana Nair ·  
Hongho Kim · Elizabeth Cha · Martin Curry · Lee Akst · Rex Yung ·  
Jeremy Richmon · Russell Taylor

Received: 15 September 2011 / Accepted: 12 November 2011 / Published online: 27 December 2011  
© Springer-Verlag London Ltd 2011

**Abstract** This paper describes the continued development of the Robotic EndoLaryngeal (Robo-ELF) Scope System, a simple clinically usable robot for manipulating flexible endoscopes, particularly in laryngeal surgery. The system includes a robot with three active and two passive degrees of freedom, a five degree of freedom passive positioning arm, a malleable scope shaft support, and a custom joystick controller. The Robo-ELF Scope allows a surgeon to control a flexible endoscope with only one hand and also to release the controls and perform bimanual surgery if desired. We have evaluated the Robo-ELF Scope system in both phantom and cadaver studies and found it superior to hand manipulation of flexible endoscopes and conventional rigid endoscopes.

**Keywords** Laryngeal surgery · Robotic surgery · Endoscope manipulation · Flexible endoscope · Endoscopic surgery

### Introduction

There has recently been a significant movement in laryngeal surgery toward transoral endoscopic surgery. While transoral endoscopic surgery reduces the risk of complications, such as scarring and infection, by utilizing natural orifices, it also presents significant surgical challenges, particularly poor sensory feedback, reduced visibility, limited working area, and increased hand tremor due to long instruments [1].

Several robotic surgical systems, most notably Intuitive Surgical's da Vinci, have sought to remedy these problems in other surgical venues, but these solutions do not transfer well to laryngeal surgery. The da Vinci was designed primarily for robotic laparoscopic surgery, in which instrument position and orientation simulate the normal hand position of a surgeon, with widely-spaced, large-diameter instruments. The result is a large, bulky robot which can be difficult to work around and which can cause additional problems with intubation for general anesthesia when instruments limit access to the airway [2]. In transoral laryngeal surgery, this approach has further limitations, since access through the airway requires nearly parallel instrument shafts, which the da Vinci cannot achieve. To partially compensate for these shortcomings, such systems often require highly modified surgical techniques and specialized clinical equipment, resulting in the need for extensive additional training for surgeons and prohibitively high startup and maintenance costs [3].

---

The original work published in The Hamlyn Symposium on Medical Robotics 19–20 June, 2011.

---

K. Olds (✉) · J. Kriss · A. Nair · H. Kim · E. Cha · R. Taylor  
Engineering Research Center for Computer  
Integrated Surgical Systems and Technology,  
Johns Hopkins University, 3400 N. Charles Street,  
Baltimore, MD 21218, USA  
e-mail: kolds1@jhu.edu

A. Hillel · M. Curry · L. Akst · J. Richmon  
Department of Otolaryngology, Head and Neck Surgery,  
Johns Hopkins Hospital, 601 N. Broadway,  
Baltimore, MD, USA

R. Yung  
Department of Pulmonology, Johns Hopkins Hospital,  
Baltimore, MD, USA

Another approach partially actuates a flexible endoscope for diagnostic use in the nasal cavity. This approach uses a two degree of freedom hand-held manipulator which controls scope rotation and tip angle—but not translation, which is left for the surgeon to control manually. This system is small and simple, overcoming many of the problems faced by more complex systems like the DaVinci, but since the scope is not completely robotically controlled, its benefits during surgery are limited [4].


Outside of robotic systems, the current state of the art in laryngeal surgery makes heavy use of rigid endoscopes. Flexible scopes are frequently used in the clinic for diagnostic procedures and an increasing breadth of therapeutic ones. Current clinical endoscopes are very advanced, offering HD video, working ports, high range of motion tips, and full sterilizability. However, the way endoscopes are currently used has many drawbacks. In a typical procedure, one surgeon holds and actuates the endoscope, which requires both hands, while another uses instruments, such as forceps and a laser, to manipulate and ablate tissue. This leads to a crowded working environment with two surgeons crowded around the patient. We also found that coordination between the two surgeons can be difficult and that supporting and actuating the endoscope for long periods of time can result in fatigue and inaccuracy.

## Methods

### System overview

We propose a relatively simple, small, inexpensive robot that takes full advantage of existing clinical equipment with the goal of using this technology in the operating room (OR) on anesthetized patients. We focused on developing a robot to hold and actuate an unmodified clinical endoscope, allowing one surgeon to control the scope with one hand using a custom-made joystick console and to operate with the other hand, or to position the scope using the robot, then operate bimanually. We used the Pentax VNL-1570STK flexible laryngoscope in these experiments, but the system is designed so that any similar clinical endoscope could be used with minimal modification. We have also developed a prototype to allow for manipulation of much longer scopes (gastroscope, colonoscope, etc.) by feeding the scope shaft independently of the scope body.

We found that surgeons generally use three degrees of freedom when manipulating flexible endoscopes: bending of the scope's tip using the scope handle, rotation of the scope about its axis, and translation of the scope along the axis of the airway; therefore, these are the degrees of freedom that the Robo-ELF has active control over. To aid in positioning the scope and in scope removal, in the case of

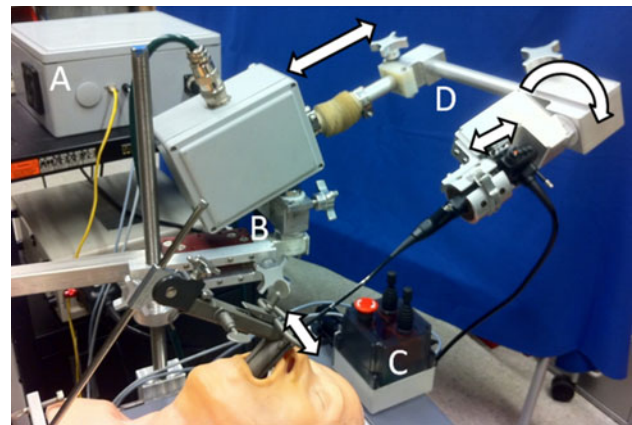

**Fig. 1** Robotic EndoLaryngeal (Robo-ELF) Scope System. A Electronics enclosure, B five degree of freedom positioning arm, C joystick enclosure, D robot system



**Fig. 2** The malleable support allows the scope shaft to stand up against gravity

emergency, we also added two passive lockable degrees of freedom to the robot itself, as well as a five degrees of freedom to the passive positioning arm (Fig. 1). To further aid in controlling the scope, we have experimented with malleable scope stiffening supports (Fig. 2). The system is currently controlled using a custom joystick interface, but we have also investigated more sophisticated image guidance techniques. The system also incorporates numerous overlapping hardware and software safety features to ensure that no single fault in the system can result in patient injury.

### Robot

In order to minimize weight over the patient, we designed the system so that the largest motors, those designed for the scope translation and rotation degrees of freedom, are located in the main box. To transmit power from the main box to the scope rotation joint, we used a cable-pulley mechanism and 12 V servo motors with planetary gearheads and integrated magnetic encoders for all active degrees of freedom. We also installed potentiometers on each active degree of freedom for added safety. Motor control is achieved using a Galil DMC-4030 with built-in 1A linear amplifiers. Potentiometer signals are buffered and lowpass filtered before digitalization using the Galil controller's built-in analog/digital conversion.

The robot grips the scope with custom-molded urethane rubber inserts and uses a quick release latch to hold the scope in place. This allows for rapid removal of the scope in case of emergency. Both active and passive robot joints are sealed with corrosion-resistant sealed bearings, o-rings, or bellows, allowing the robot to remain fully watertight even when in motion. The electrical connection to the robot is achieved using a Soriau corrosion-resistant waterproof electrical connector. All compartment covers are sealed with o-rings.


The entire robot is built with Johns Hopkins Hospital clinical engineering specifications in mind, including waterproof seals, OR-safe materials, proper electrical grounding with fusing, and an isolated power supply with no voltages greater than 12 V. The robot is operable in wet environments and is awaiting a final clinical engineering inspection.

### Positioning arm

The robot is positioned using a five degree of freedom passive lockable positioning arm (Fig. 1). This allows the surgeon to quickly and easily position the robot with respect to the patient, as well as quickly move the robot in case of emergency. We used a five degree of freedom design in order to capture all of the degrees of freedom that we observed surgeons using in the OR. These include (1) horizontal translation of the scope in order to account for patient position, (2) vertical translation of the scope to adjust to surgeons of different heights and different patient positions, (3) axial translation of the scope to allow for quick and easy insertion to the vicinity of the surgical target, (4) rotation of the scope about the vertical axis to correct for patient misalignment, and (5) rotation of the scope about the horizontal axis to angle the robot's active translation degree of freedom for optimal insertion into the laryngoscope. All degrees of freedom are lockable using a screw-driven shaft collar design controlled using large knobs in order to facilitate use when wearing gloves and in wet environments. All joints use low-friction plastic washers both to prevent wear/dust creation and to provide smooth motion.

Some degrees of freedom could present possible danger to the patient or surgeon when they are unlocked, since the weight of the robot could cause the joint to suddenly move. We therefore added adjustable plastic friction collars to the two degrees of freedom which were affected (robot rotation about the horizontal axis, and the robot arm's elbow rotation). The friction collars prevent these joints from moving under their own weight, thus improving safety.

Two passive degrees of freedom are also particularly important for emergency scope removal. The first is the robot's elbow joint, which allows the whole robot arm to be

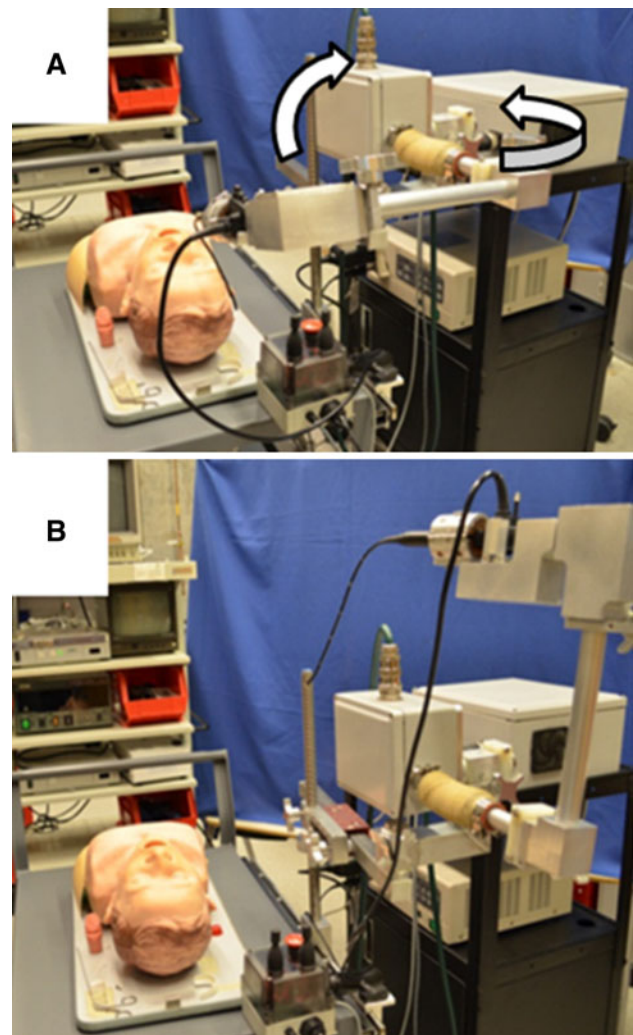


**Fig. 3** The scope can be quickly removed from the vicinity of the patient by using the passive elbow joint on the robot arm. **a** Rotate the knob and raise the arm. **b** The arm has been raised

quickly rotated out of the vicinity of the patient (Fig. 3). The second is the passive positioning arm's axial translation degree of freedom, which allows the scope to be quickly manually withdrawn from the patient's mouth. It is up to the surgeon's judgment which removal method is most appropriate given the location of the scope with respect to the patient's anatomy.

### Joystick

We originally used a 3DConnexion Space Navigator 3D mouse to control the robot, but this device presented many difficulties in this application. With a three-dimensional (3D) mouse, it proved difficult to separate the different degrees of freedom when operating the robot, for example, to only actuate the scope handle without also moving the scope in other ways. The 3D mouse was also prone to slipping, dropping, and bumping in a chaotic OR environment,



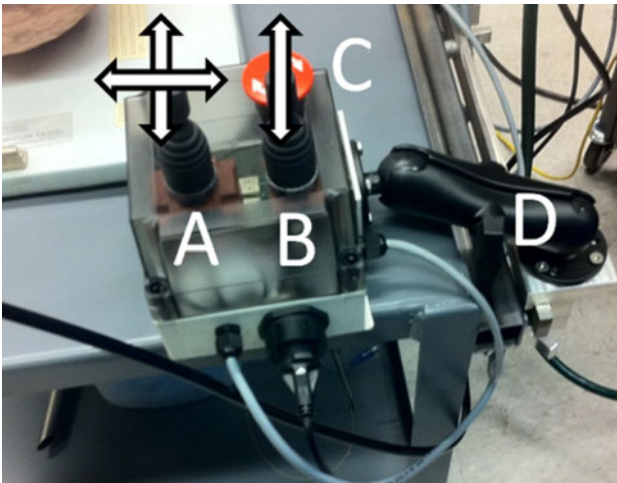

**Fig. 4** Joystick enclosure. *A* Two degree of freedom joystick, *B* one degree of freedom joystick, *C* emergency off button, *D* joystick positioning arm

and has no resistance to liquids. This led us to use a control strategy that relies on custom joysticks which can only be active in one direction at a time (Fig. 4). This completely separates the robot degrees of freedom, allowing for much more precise control. To avoid sliding and falling in the OR, the joystick can be anchored to the bed rail using an adjustable arm. The joystick enclosure also includes an emergency stop button in case of emergency. The joystick enclosure is sealed with all waterproof and corrosion-resistant connectors and components and can be wiped down with standard hospital grade cleaners.

In order to provide even greater safety, the joystick system was designed so that each joystick degree of freedom controls two independent electrical switches. For example, when the joystick is pushed forward, the forward switch is turned on, and the reverse switch is turned off. This redundancy allows for greater error checking and also prevents small incidental movements of the joystick from moving the robot, since the joystick needs to be fully deflected in order for the switches to activate.

One disadvantage of this on–off control style is that it can lead to jerky movement of the robot. To counter this, we added speed ramp-up functionality to the robot control software, which allows the robot to increase its velocity (up to a pre-determined maximum velocity) the longer the joystick is held. The end result is that for long motions, the joystick can be held and the robot will ramp up to speed in seconds, but for short, delicate motions, short joystick movements result in slow, controlled motion.

#### Safety systems

The Robo-ELF incorporates layers of overlapping safety systems to ensure that no single failure in the system can

result in patient injury. The most basic safety feature is the manual emergency stop button on the joystick enclosure, which allows the surgeon to directly cut the power to the motors at any time. In series with the emergency button is a computer controlled USB relay, which allows the robot control computer to automatically cut motor power if it detects any problems with the motor controller or other systems.

The motor controller and PC also have a two-way software heartbeat function, so that if either encounters problems, or the connection is cut, the system will be able to respond by shutting off the motor power. Another layer of software safety is added by using a position control scheme, in which only very small incremental position commands are sent to the motor controller. In case of a failure in the connection that the heartbeat does not catch, the robot will simply stop at the next position increment. This is contrasted with velocity control, where the robot would continue at its last commanded velocity.

In order to aid in fault detection, all active joints on the robot use redundant sensors. The motors have integrated magnetic encoders, and the joints all have independent potentiometers directly coupled to the joints themselves. This results in two fully independent measurements of joint position. Also, since one measurement is digital and incremental, and the other is analog and absolute, it is unlikely that any single fault could result in undetected joint position errors.


The electrical power system also incorporates several safety features, including fusing on the main power supply, grounding of the entire robot case to earth ground, and a 12 V isolated DC power supply. These features ensure that no voltage outside of the AC/DC converter exceeds  $\pm 12$  V.

#### Scope support

The scope shaft is highly flexible, so we added a malleable wire scope shaft support to stiffen it for more precise control (Fig. 2). This combines the easy controllability of a rigid endoscope with the flexibility and safety of a flexible endoscope. Making the scope motion more predictable by stiffening the shaft also greatly simplifies the control of the scope, which is useful in both manual robot control and automated image-based scope control.

#### Evaluation

Our surgeon co-authors (Drs. Akst, Hillel, and Richmon) have tested the system using two fresh human male cadavers. We suspended each cadaver with a Steiner laryngoscope to allow visualization of the endolarynx, in a configuration similar to (Fig. 5). First, we performed standard microlaryngoscopy using  $0^\circ$ ,  $30^\circ$ , and  $70^\circ$  rigid

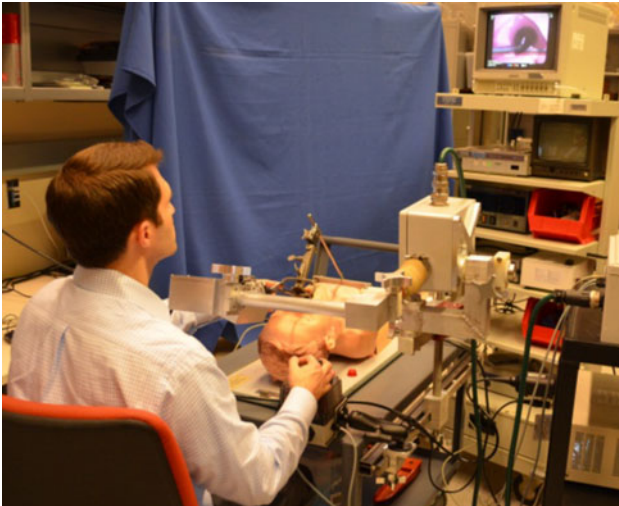

**Fig. 5** Dr. Richmond evaluating the Robo-ELF Scope system with the rubber head and neck phantom

scopes, taking representative photographs of the endolarynx with each scope for comparison. We then evaluated the Robo-ELF with the following three tasks: (1) comparable field of view, (2) visualization of challenging anatomical areas with precise biopsy sampling; (3) bimanual surgery with the Robo-ELF in a fixed position.

We also conducted an evaluation of the current system using a rubber head and neck phantom. This evaluation focused on both testing the robot's systems, and getting qualitative feedback from surgeons.

## Results

### Cadaver study

This study was conducted before the introduction of the custom joystick system, and the five degree of freedom positioning arm, so the robot was clamped to a surgical table for the experiments. Using the passive degrees of freedom of the robot, we easily positioned the Robo-ELF through the Steiner laryngoscope. All three active degrees of freedom performed reliably, with smooth, consistent, reproducible motion. The velocity of the movement was reliably transmitted through motion of the 3D mouse, with no erratic artifacts and virtually no learning curve. The Robo-ELF provided a higher resolution image with superior field of view compared to the three rigid endoscopes. In addition, we were able to navigate the flexible tip around the arytenoids into the piriform sinuses, and through the vocal cords into the subglottis, overcoming the line of site limitations of rigid scopes. Although we were able to visualize the intended biopsy sites in both cadavers, the first cadaver's larynx was anteriorly positioned, so despite

obtaining a clear view of the subglottis and anterior commissure with the Robo-ELF in a flexed position, the straight laryngoscopic forceps were unable to reach it. Finally, after positioning the Robo-ELF above the vocal cords there was still ample room to use two instruments to perform bimanual endolaryngeal surgery [5].

### Phantom evaluation

We placed the phantom on a mock surgical bed (Fig. 5), suspended it using a Steiner laryngoscope, and attached the robot to the bed rail. The robot was positioned using both its passive degrees of freedom and the five degree of freedom positioning arm. The scope video stream was displayed on a standard surgical video display. The surgeons then attempted to navigate through the phantom using the joystick controls, testing responsiveness, ability to reach desired targets, and ease of use. Surgeon feedback was generally positive, and the joystick system was vastly preferred over the 3D mouse.

## Discussion

The technological advantages of this approach are substantial. This robot is inexpensive compared with other microscopic and robotic techniques, at approximately \$30,000. On top of this platform, we also plan to integrate more sophisticated software features, including automated scope stabilization, 3D reconstruction from multiple monoscopic scope images, automated point-and-click navigation, video registration with pre-operative imaging data, and virtual fixtures. We have already begun investigation two additional features, image-based navigation, and manipulation of longer endoscopes, using the Robo-ELF as a base.

We have examined several strategies to augment the control of the robot with image-based feedback. The most promising so far is a point and click style interface, where the surgeon uses a touch screen or a mouse to "click" on the image where he/she wants the scope to point. The robot would then use a kinematics-based control strategy, with visual feedback to correct for errors in the kinematic estimate. We conducted a phantom evaluation of this method, but it proved difficult to implement with template matching because of the poor texture and high specularly in the larynx (of both cadavers and our phantom). However, we plan to investigate more sophisticated vision methods (SLAM, etc.) to resolve these problems.

The Robo-ELF's 10-cm insertion/extraction degree of freedom is insufficient for use with longer endoscopes, such as bronchoscopes. Bronchoscopic procedures often require intricate navigation over a range up to 40 cm. One solution we considered was to extend the range of the Robo-ELF,

but we found that this solution becomes impractical with longer endoscopes. Instead, we developed a prototype scope shaft manipulation system that manipulates the scope shaft independently of the scope body. This method allows for coarse feeding of long scope shafts until they are in the desired location, while still maintaining the fine motion of the Robo-ELF's translation stage during surgery. This prototype has been tested independently using a standard clinical bronchoscope, but has not yet been integrated with the rest of the Robo-ELF system.

The Robo-ELF could also be utilized with other technology, such as image-overlay, ultrasound, and optical coherence tomography, and be manufactured with two chips for 3D vision. Furthermore, it could be adapted to a variety of procedures, including bronchoscopy, upper and lower gastrointestinal endoscopy, and sinus surgery. Eventually there is potential for microvascular surgery at the base of the skull, as well as single port gastrointestinal and thoracic access surgery. The flexible endoscope also has a working channel through which a therapeutic laser could be introduced, further taking advantage of standard clinical equipment.

## Conclusion

We have shown that a relatively small, inexpensive three degree of freedom robot can be used to precisely control an

unmodified clinical endoscope with virtually no learning curve. The Robo-ELF has demonstrated significant advantages over existing robotic surgery systems, as well as un-actuated rigid and flexible endoscopes in the field of laryngeal surgery.

**Acknowledgments** Funding was provided by Johns Hopkins Hospital Department of Otolaryngology Internal Funds. REU Site for Computational Sensing and Medical Robotics Award Number 1,004,782.

**Conflicts of interest** None.

## References

1. Plinkert P, Lowenheim H (1997) Trends and perspectives in minimally invasive surgery in otorhinolaryngology-head and neck surgery. *Laryngoscope* 107:1483–1489
2. Lee H, Yun M, Bahk J, Park H, Jeon Y, Lee S (2010) Rupture of endotracheal tube cuff during robot-assisted endoscopic thyroidectomy. *Korean J Anesthesiol* 59(6):416–419
3. McLeod IK, Mair EA, Melder PC (2005) Potential applications of the da Vinci minimally invasive surgical robotic system in otolaryngology. *Ear Nose Throat J* 84:483–487
4. Eckl R, Gumprecht J, Strauss G, Hofer M, Dietz A, Lueth T (2010) Comparison of manual steering and steering via joystick of a flexible Rhino endoscope. In: 32nd annual international conference of the IEEE, Engineering in Medicine and Biology Society (EMBC), Buenos Aires, pp 1234–1237
5. Olds K, Hilel A, Cha E, Curry M, Akst L, Richmon J, Taylor R. Robotic endo-laryngeal flexible (Robo-ELF) scope: a preclinical feasibility study. *Laryngoscope* (in press)